



# The Open Public Health Journal

Content list available at: <https://openpublichealthjournal.com>



## RESEARCH ARTICLE

# Combating the COVID-19 Pandemic Using 3D Printed PPE: Challenges and Recommendations

Amaar Amir<sup>1\*</sup> and Baraa Amir<sup>1</sup>

<sup>1</sup>Imam Abdulrahman Bin Faisal University, Dammam, Saudi Arabia

### Abstract:

#### Background:

The World Health Organization declared COVID-19 a pandemic in March of 2020. As traditional respiratory personal protective equipment (PPE) was in severe shortage, communities turned to 3D printing to provide printed PPE alternatives; however, certain hurdles need to be addressed to ensure the safety of users.

#### Objective:

One main consideration when dealing with 3D printed parts is the presence of pores. Several studies have found the diameter of these pores to range widely from as little as 10µm to over 150 µm, making them larger than the droplets and nuclei through which the virus is transmitted.

#### Methods:

Researchers found that altering print settings, such as increasing the extrusion multiplier, may decrease the size and number of these perforating pores. Other challenges include the variable reproducibility of printed PPE, which may be remedied through printer calibration. Storage and sterilization are also a challenge as most 3D printed plastics do not tolerate disinfection methods, such as autoclaves. The use of chemical disinfectants is recommended instead. The rigidity of printed plastics may compromise the fit of masks for varying users. Using 3D scanning may provide personalized masks that seal appropriately.

#### Results:

One final issue is the prolonged interaction with 3D printers of inexperienced users, predisposing them to the respiratory tract and skin irritation; thus, adequate ventilation and protection are mandatory.

#### Conclusion:

Documenting the benefits and drawbacks of this form of PPE production carries great significance in light of the ongoing COVID-19 pandemic, as well as any future public health emergencies.

**Keywords:** 3D printing, COVID-19, Personal protective equipment, Surgical mask, N95 mask, Face shield.

### Article History

Received: January 24, 2022

Revised: January 27, 2022

Accepted: March 15, 2022

## 1. INTRODUCTION

On December 31<sup>st</sup>, 2019, clusters of pneumonia cases were reported in Wuhan, China; three months later, the novel coronavirus, COVID-19, was declared a pandemic by the World Health Organization (WHO) [1]. Due to the crushing demands, supply of traditional respiratory personal protective equipment (PPE) quickly became limited. One solution to combat this mismatch emerged in the form of 3D printed PPE. 3D printing has proved to be a suitable interim replacement in times of need due to easy access to 3D printers and design software, the abundance of material choices, and the reusability of printed parts. 3D printing has played a crucial role in fulfil-

-ling the PPE demands during shortages experienced at the beginning of the COVID-19 pandemic. According to the United States Food and Drug Administration (FDA), additive manufacturing has contributed to producing approximately 53 million PPE, PPE accessories, and medical devices [2]. Despite this, there remain challenges that need to be addressed, as cited previously in statements released by the FDA [3]: “While it is possible to use 3D printing to make certain PPE, there are technical challenges that have to be overcome.”


## 2. SYNOPSIS OF THE WIDESPREAD IMPACT OF 3D PRINTED PPE

In response to the sudden supply chain shortages of traditional PPE, non-traditional producers (NTP) were quick to design and produce 3D printed PPE in large quantities. While

\* Address correspondence to this author at the Imam Abdulrahman Bin Faisal University, Dammam, Saudi Arabia; Te: 00966541248025, E-mail: [Amaarabulrazackamir@gmail.com](mailto:Amaarabulrazackamir@gmail.com)

exact production estimates may vary, one study found that over the course of 5 months in the United States alone, 53 million 3D printed PPE and medical devices were produced utilizing more than 33,000 3D printers. The majority of printed PPE came in the form of face shields, which amounted to 38,295,580 units produced in total with a maximum daily production capacity of 502,593 units. Test swabs were the second-largest produced 3D printed medical devices with 12,376,896 total units produced and a maximum daily capacity of 948,204 units. Ear savers, masks and mask parts, and ventilator parts were the least produced items, with an estimated total production of 2,560,954 units, 241,869 units, and 116,455 units, respectively [2]. The distribution of said 3D printed PPE was in concordance with the intensity of COVID-19 infection rates in different geographical areas (Fig. 1). Examples of different recipients of printed PPE from NTPs in the United States include Massachusetts General Hospital, the Johns Hopkins Health System Corporation, Northwell Health, Seattle Children's Hospital, Novant Health, and Michigan Hospitals, among others (Fig. 2). During this time, the "NIH 3D Print Exchange" program was established wherein the National Institute of Health (NIH), United States Department of Veterans Affairs (VA), America Makes, and FDA, all participated in testing and validating various 3D designs of PPE uploaded by the community. The testing criteria used were based on an amalgamation of standards and

regulations from the FDA, Center for Disease Control, and National Institute for Occupational Safety and Health. In total, 645 designs were uploaded, with 33 and 28 designs approved for clinical use and community use, respectively [4 - 7]. 25% of NTPs used approved 3D printed PPE designs from the NIH 3D Print Exchange program making up the majority of alternative PPE produced for essential workers and healthcare personnel [2]. As such, tested and verified printed PPE had a worldwide reach with online visitors browsing the NIH 3D Print Exchange programs website from over 1000 cities across the globe (Fig. 1) [8]. Whilst initially being met with reluctance, 3D printed PPE had now started to become widely accepted in the community for a multitude of reasons. This, in part, was due to the fact that 3D printers are relatively easy to access and can produce complex geometrical shapes with a high degree of precision, and also due to their ability to use a host of different plastic filaments, which can give the PPE varying physical properties. 3D printing can also work to enhance traditional PPE, such as in the case of mask fitters and mask tensioners. 3D printed PPE is also reusable and can be disinfected more easily, unlike most traditional PPE. This is especially noteworthy as a study conducted in 2020 surveying over 23,000 nurses in the United States reported that 87% of nurses complained of having to reuse a single-use disposable mask or N95 respirator during the first couple of months of the pandemic [9].

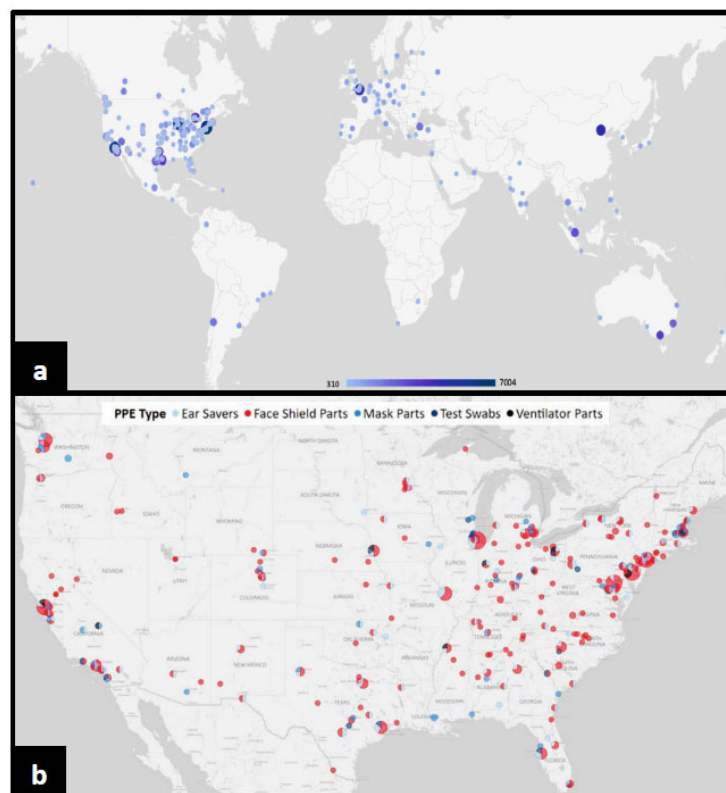

**Fig. (1).** Maps visualizing the large impact of 3D printed PPE. **a)** This map represents online visitors to the NIH 3D Print Exchange programs website with visitors from over 1000 cities being represented by colour and relative size. Some cities are grouped together for the sake of preserving good visibility and resolution. **b)** This map represents the distribution of 3D printed PPE and medical devices in the United States with face shields being the most commonly distributed item. Different cities received varying numbers of printed PPE depending on the intensity of infection rates as is represented by the relative size of the circles. Adapted from [2, 8].

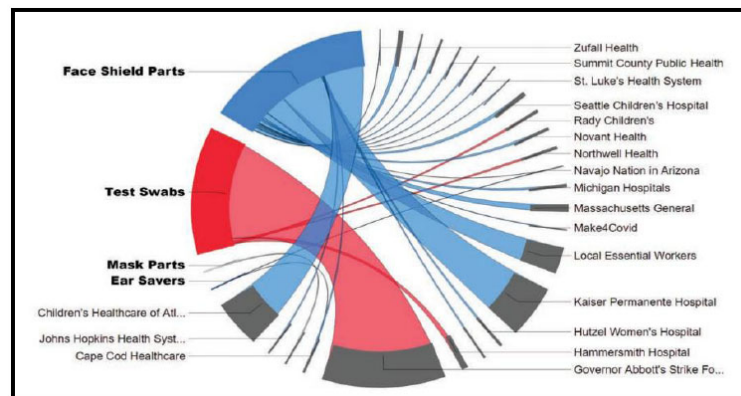


Fig. (2). Example recipients of 3D printed PPE, PPE accessories, and medical devices in the United States. Adapted from [2].

### 3. CHALLENGES AND ASSOCIATED RECOMMENDATIONS RELATED TO 3D PRINTED PPE

#### 3.1. Porosity and Mask Integrity

Fused Deposition Modelling (FDM) printers are some of the most widely used types of 3D printers in both hobbyist and commercial settings alike [10]. However, the main shortcoming of FDM printing is the relatively low production quality coupled with the porous nature of the finished print. This may be problematic when involving respiratory PPE production as pores may affect the PPE performance as air and fluid barriers. The COVID-19 virus, known as SARS-CoV-2, was found to range in diameter from  $0.065\mu\text{m}$ - $0.125\mu\text{m}$  (Fig. 3) [11, 12]. Although, worth noting is that the virus particles, as reported by the WHO, are transmitted primarily through respiratory droplets ranging in size between  $5\mu\text{m}$ - $10\mu\text{m}$ . The WHO also reported the potential of transmission through airborne nuclei  $<5\mu\text{m}$  in specific settings, such as aerosol-generating procedures or in small, indoor, and poorly ventilated areas [13]. One study found that objects printed with FDM printers contain chaotically arranged pores averaging in size approximately between  $10\mu\text{m}$ - $20\mu\text{m}$ , making them larger than the virus-containing droplets and nuclei [14]. The researchers of the said study were then able to alter the porosity by

readjusting printing parameters, such as increasing the extrusion multiplier, allowing for internal filling of the printed walls and distribution of seams for each layer in random positions. Increasing the extrusion multiplier showed to have the largest effect on the porosity of the printed parts. After analysing the modified parts via a scanning electron microscope (SEM), the researchers revealed a reduction in pore size and the absence of any perforating pores (Fig. 4). This provides promising data in the search to eradicate pores in printed parts. However, the researchers indicated varying results depending on the different geometry of the 3D printed components (Fig. 5). Simple geometrical shapes were tested and displayed selected areas of increased porosity. Despite the availability of such data, reducing porosity in complex shapes, such as face masks, may yet be challenging. Another study concerning a different method of 3D printing termed Selective Laser Sintering (SLS) also found the presence of pores. These pores ranged in size from  $15\mu\text{m}$ - $150\mu\text{m}$  [15]. This study did not conduct a follow-up test after adjusting the print settings. The pores in the 3D printed material in both studies were significantly larger than those found in a variety of traditional PPE, such as certified N95 masks, which are rated at  $0.3\mu\text{m}$  [16]. However, this porosity may not be of great concern in regards to PPE used in environments where airborne-precautions do not apply such as in community settings and non-specialized clinical settings (Fig. 6).



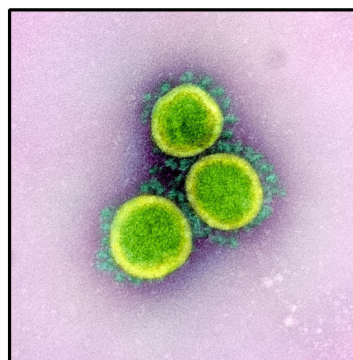


Fig. (3). Transmitting electron microscope image showing SARS-CoV-2 virus particles after being isolated from a patient. The image displays spike proteins on the outer edge of the virus particles which give the coronaviruses their name; "crown-like". Image captured and colour-enhanced at the National Institute of Allergy and Infectious Diseases' Integrated Research Facility in Fort Detrick, Maryland. Adapted from [12].

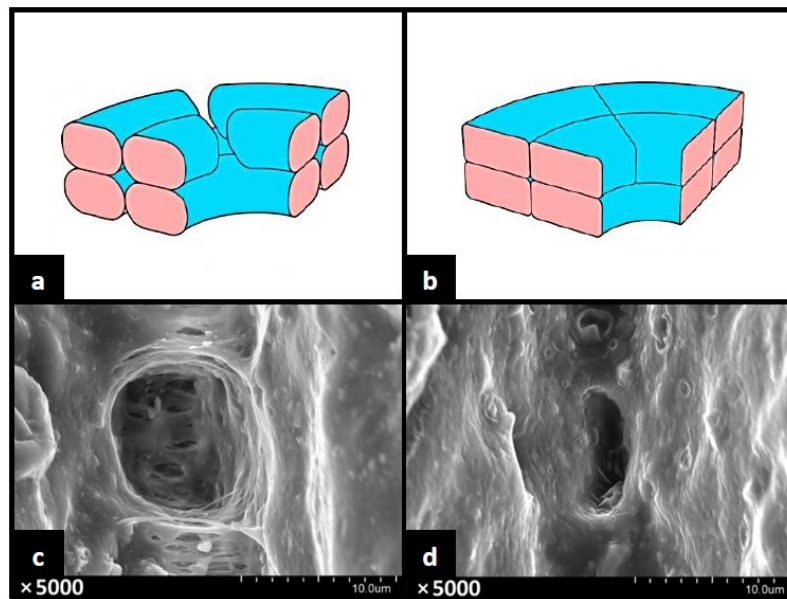

**Fig. (4).** Digital renders and scanning electron microscope (SEM) images showing the effect of the extrusion multiplier setting on porosity. **a)** Digital render with low extrusion multiplier showing gaps. **b)** Digital render with high extrusion multiplier showing smaller gaps. **c)** SEM images with low extrusion multiplier showing large pores. **d)** SEM images with high extrusion multiplier showing smaller pores. Adapted from [14].

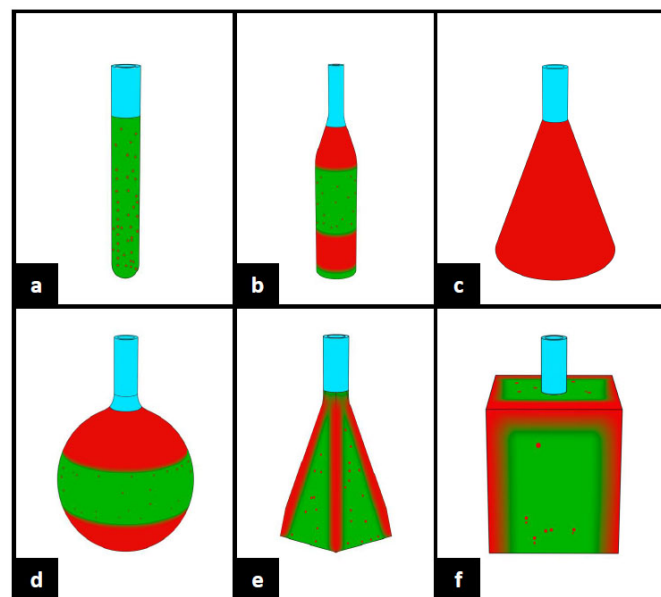

**Fig. (5).** Digital renders showing the different effects of the extrusion multiplier setting on porosity in different geometric shapes. Areas in red indicate high porosity, and areas in green indicate relative impermeability. **a)** Cylinder; **b)** Compound shape; **c)** Cone; **d)** Sphere; **e)** Pyramid; **f)** Cube. Adapted from [14].

### 3.2. Variable Reproducibility

Despite the fact that the digital and downloadable standard tessellation (STL) files of 3D printed PPE do not differ from one computer to another in terms of printing, these STL files will, more often than not, result in printed PPE with slightly varying dimensions across different 3D printers. This is due to dissimilar printer calibration levels as well as small differences in the generated g-code from different slicing software and

print settings. The end result may be an aesthetically similar, but functionally different set of PPE [17]. Furthermore, varying materials may also increase functional differences in the printed products. This lack of quality control was stated as a significant reason behind the inability to ensure the quality, safety, and efficacy of 3D printed PPE by the NIH, VA, and FDA [18]. As such, it is recommended to ensure adequate printer calibration and adhere to the print settings suggested by the original designer of any proficient 3D printed PPE model.


### 3.3. Heat Sensitivity and Sterilization

FDM printing involves a wide selection of thermoplastic filaments, with polylactic acid (PLA) being a popular choice among the users. This is due to its cost-efficiency, widespread availability, and high print success rates when using basic 3D printers with and without heated build plates. However, printed PLA components are more sensitive to heat compared to other printed plastics. While PLA does have a melting temperature between 130°C – 180°C, the glass transition temperature for amorphous PLA lies only between 55°C – 60°C, wherein the plastic becomes soft and may warp [19]. This glass transition temperature increases slightly in semicrystalline PLA. This property of PLA is especially problematic for common hospital sterilization methods involving high temperatures, such as using dry heat and autoclaves, which regularly operate at 121°C or 132°C [20]. The WHO, therefore, recommends sterilization of plastic respiratory equipment that may not tolerate high temperatures, such as PLA printed PPE, by using chemical disinfectants and soaking in a 0.1% sodium hypochlorite solution for most cases. For cases of equipment exposed to over 10ml of blood or body fluid, a higher concentration of 0.5% is recommended [21 - 23]. Such chemical disinfectants require cautious use to avoid wear on the printed PPE.


### 3.4. Ergonomics and Seal

While alternative plastics may overcome the aforementioned temperature barriers, they still share other

drawbacks with PLA printed PPE, such as the inability to readily conform to different facial features. This may not greatly affect printed face shields; however, it will likely have a significant effect on printed masks as said masks may fail fit tests when worn by different individuals. This nullifies the mechanical filtration of the printed mask to a degree as air will pass through the gaps between the mask and the face of the user and avoid the higher resistance filter. Additionally, this may make wearing a printed PPE uncomfortable for certain individuals. Hobbyists have recommended using flexible plastics, such as thermoplastic urethane (TPU) and thermoplastic elastomer (TPE), although these materials have an equally low glass transition temperature to PLA making them difficult to sterilize. Comfort foam inserts may be inserted into the posterior aspect of printed masks to accommodate different facial features. One innovative solution came in the form of the Bellus3D Mask Fitter, which involves scanning the face of the user through a mobile application and providing an STL file for a mask frame that is individually contoured and can be printed (Fig. 7) [24]. This will likely improve the seal of certain masks, as was evident in a study conducted in an ophthalmology setting during the COVID-19 pandemic. The study recruited 20 individuals who used a level 3 fluid resistant face mask with a 3D printed mask fitter on top in an effort to simulate N95 respirators. 90% of the participants (18 out of 20) successfully passed the fit test with only minor complaints regarding ease of use and comfort. This study provided a case for how 3D printing can augment traditional PPE performance [25].

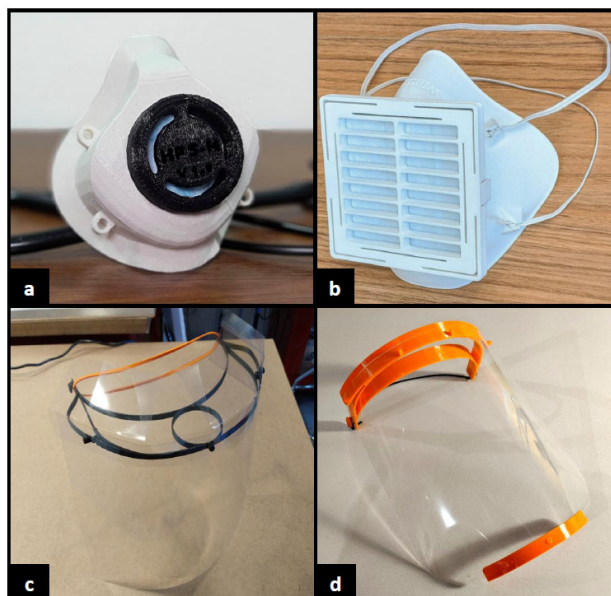

**Fig. (6).** Examples of 3D printed mask and face shield designs tested by the NIH, VA, and FDA. **a)** Community Face Mask; a cloth mask-alternative deemed suitable for use in the community during the COVID-19 pandemic. **b)** Stopgap Surgical Face Mask (SFM) Revision B; a surgical mask deemed suitable for clinical use during the COVID-19 pandemic. **c)** Minimum Viable Product Face Shield v1; a face shield deemed suitable for use in the community during the COVID-19 pandemic. **d)** Prusa Protective Face Shield RC3 US version; a face shield deemed suitable for clinical use during the COVID-19 pandemic. Adapted from [4 - 7].

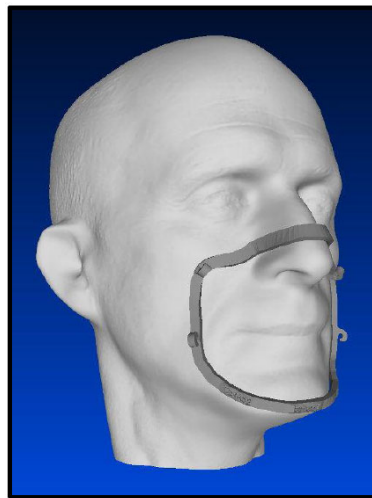

**Fig. (7).** Digital render of the Bellus3D Mask Fitter which can be worn over masks to improve the seal. The design of the Mask Fitter is generated by using a facial scan of the user and creating the appropriate corresponding geometry. This concept is deemed suitable for clinical use during the COVID-19 pandemic by the NIH, VA, and FDA. Adapted from [24].

### 3.5. Health Considerations

FDM 3D printers carry varying levels of health risks for users depending primarily on the type of plastic filaments utilized. Acrylonitrile butadiene styrene (ABS) plastics have been well documented to release larger amounts of Volatile Organic Compound (VOC) thermal decomposition products during printing when compared to PLA and other filaments. In total, nearly 216 VOCs were identified, many of which are carcinogenic. Reports also indicate a 33%-38% increase in airborne particle concentration after printing with ABS compared to PLA [26]. Regardless of the filaments used, almost all 3D printers release ultrafine particles (UFP), which pose a health risk to those chronically exposed. UFPs pose an increased risk for respiratory complications compared to fine particles as they are smaller in size and possess a larger surface area. As such, if UFPs are present in the lungs, they remain longer and tend to cause increased levels of inflammation, which manifest as cough and deteriorating shortness of breath [27]. Several studies have documented the onset of asthma in users heavily exposed to 3D printers. One such study surveyed multiple Canada-based companies, whose workers utilized 3D printing heavily as part of their normal workflow. 46 workers were surveyed in total, 27 of which complained of respiratory symptoms at least once weekly in the past year. The researchers concluded that exposure to operating 3D printers for over 40 hours weekly statistically significantly increased the likelihood of suffering from respiratory-related diseases, such as asthma and allergic rhinitis [28]. This is especially of interest in the context of PPE production during the COVID-19 pandemic, as many unexperienced individuals may obtain and run 3D printers with no hindsight of such potential health implications. Individuals wishing to print and distribute copious amounts of PPE may not have adequate safety equipment and work settings. It is therefore recommended to decrease exposure whenever possible to operating 3D printers and provide adequate ventilation and protective equipment to those interacting with the printers. Worth noting is that most

studies conducted analyse the harms of 3D printing during the active process of printing, which involves melting plastics and releasing hazardous fumes and particles. However, another less researched area of interest is the possible biocompatibility issues of using 3D printed plastics as PPE. Biocompatibility depends on a host of factors, including duration and type of contact [29], as well as the nature of any trace materials in the printed product. One study conducted in 2021 investigated 24 traditional surgical and KN95 masks for toxic substances. Most of the masks tested contained trace elements below their corresponding detection thresholds; however, selected number of masks contained detectable amounts of trace elements. Examples of elements found were Pb, Cu, Zn, and Sb [30]. These potentially hazardous elements could be transferred to the user via a process called metal leaching, wherein the metals would dissolve from their natural ores into a liquid medium [31]. In this case, it is likely that leaching would be triggered by exposure to human saliva, such as in the case of prolonged mask usage, chewing on the mask, or violent sneezing. In the case of 3D printed PPE, selecting specific plastics may not entirely assure suitable biocompatibility as the process of additive manufacturing may modify the properties of said plastic used [32]. There has yet to be any formal testing for trace elements in 3D printed masks and other PPE. Conducting such a test in the future could potentially aid in identifying trace elements in printed products and their sources, allowing to avoid exposure to such elements.

### CONCLUSION

While there are still some considerations that need to be addressed to ensure the safe and efficacious use of printed PPE, there is no doubt that many hospitals and communities alike have benefited from consuming 3D printed masks and face shields, particularly during the beginning of the pandemic. Additive manufacturing has aided in fulfilling the PPE demands during times of shortage, wherein tens of millions of additively manufactured face shields and hundreds of thousands of respirator and mask components were produced

and distributed. While traditional PPE stocks have since recovered, it is of paramount importance to continue research and development into 3D printed PPE in order to create safer and more efficacious equipment that can equally match, or perhaps even supersede, traditional PPE. Some organizations, such as America Makes, have recommended further testing and validation of printed PPE in order to create a digital stockpile of vetted designs, which will be available on standby in cases of any future emergency circumstances. Documenting all of the aforementioned benefits and highlighting some possible drawbacks of this form of PPE production carry great significance considering the ongoing COVID-19 pandemic, as well as in case of any future public health emergencies.

#### LIST OF ABBREVIATIONS

<b>ABS</b>	=	Acrylonitrile Butadiene Styrene
<b>FDA</b>	=	Food and Drug Administration
<b>FDM</b>	=	Fused Deposition Modelling
<b>NIH</b>	=	National Institute of Health
<b>PLA</b>	=	Polylactic Acid
<b>PPE</b>	=	Personal Protective Equipment
<b>SEM</b>	=	Scanning Electron Microscope
<b>SLS</b>	=	Selective Laser Sintering
<b>STL</b>	=	Standard Tessellation Files
<b>TPE</b>	=	Thermoplastic Elastomer
<b>TPU</b>	=	Thermoplastic Urethane
<b>UFP</b>	=	Ultra Fine Particles
<b>VA</b>	=	Veterans Affairs
<b>VOC</b>	=	Volatile Organic Compounds
<b>WHO</b>	=	World Health Organization

#### AUTHORS' CONTRIBUTIONS

AA participated in developing the study concept and design, and drafted the article. BA also participated in developing the study concept and design, and substantively reviewed and modified the drafted article. All authors read and approved the final manuscript.

#### CONSENT FOR PUBLICATION

Not applicable.

#### FUNDING

None.

#### CONFLICT OF INTEREST

The authors declare no conflict of interest financial or otherwise.

#### ACKNOWLEDGMENTS

Declared None.

#### REFERENCES

- [1] Archived. Who timeline - covid-19. World Health Organization World Health Organization <https://www.who.int/news/item/27-04-2020-who-timeline---covid-19>
- [2] Assessing the role of additive manufacturing in support of the U.S. COVID-19 response [Internet]. advanced manufacturing crisis production response (AMCPR) FDA 2021. <https://www.fda.gov/media/150614/download>
- [3] Center for Devices and Radiological Health. 3D printing of medical devices and accessories during COVID-19. U.S. Food and Drug Administration. FDA 2022. <https://www.fda.gov/medical-devices/coronavirus-covid-19-and-medical-devices/3d-printing-medical-devices-accessories-components-and-parts-during-covid-19-pandemic>
- [4] Community face mask. National Institutes of Health US Department of Health and Human Services; [cited 2022Feb3] 2022. <https://3dprint.nih.gov/discover/3dpx-013677>
- [5] Stoppag surgical face mask (SFM) revision B. National Institutes of Health US Department of Health and Human Services 2022. <https://3dprint.nih.gov/discover/3dpx-014168>
- [6] 6. Prusa protective face shield RC3 US version. National Institutes of Health US Department of Health and Human Services 2022. <https://3dprint.nih.gov/discover/3dpx-013409>
- [7] Minimum viable product face shield V1. National Institutes of Health US Department of Health and Human Services 2022. <https://3dprint.nih.gov/discover/3dpx-013403>
- [8] McCarthy MC, Di Prima MA, Cruz P. Trust in the Time of Covid-19: 3D Printing and Additive Manufacturing (3DP/AM) as a Solution to Supply Chain Gaps. *NEJM Catalyst innovations in care delivery* 2021.
- [9] New survey of nurses provides frontline proof of widespread employer, government disregard for nurse and patient safety, mainly through lack of optimal PPE. *National Nurses United* 2020. <https://www.nationalnursesunited.org/press/new-survey-results>
- [10] Dudek P. FDM 3D printing technology in manufacturing composite elements. *Arch Metall Mater* 2013; 58(4): 1415-8. [<http://dx.doi.org/10.2478/amm-2013-0186>]
- [11] Shereen MA, Khan S, Kazmi A, Bashir N, Siddique R. COVID-19 infection: Origin, transmission, and characteristics of human coronaviruses. *J Adv Res* 2020; 24: 91-8. [<http://dx.doi.org/10.1016/j.jare.2020.03.005>] [PMID: 32257431]
- [12] New images of novel coronavirus SARS-COV-2 now available. National Institute of Allergy and Infectious Diseases US Department of Health and Human Services 2022. <https://www.niaid.nih.gov/news-events/novel-coronavirus-sarsco-v2-images>
- [13] Transmission of SARS-COV-2. Implications for infection prevention precautions World Health Organization World Health Organization 2022. <https://www.who.int/news-room/commentaries/detail/transmission-of-sars-cov-2-implications-for-infection-prevention-precautions>
- [14] Gordeev EG, Galushko AS, Ananikov VP. Improvement of quality of 3D printed objects by elimination of microscopic structural defects in fused deposition modeling. *PLoS One* 2018; 13(6): e0198370. [<http://dx.doi.org/10.1371/journal.pone.0198370>] [PMID: 29879163]
- [15] Rendeki S, Nagy B, Bene M, *et al.* An overview on personal protective equipment (PPE) fabricated with additive manufacturing technologies in the era of COVID-19 pandemic. *Polymers (Basel)* 2020; 12(11): 2703. [<http://dx.doi.org/10.3390/polym12112703>] [PMID: 33207712]
- [16] Qian Y, Willeke K, Grinshpun SA, Donnelly J, Coffey CC. Performance of N95 respirators: Filtration efficiency for airborne microbial and inert particles. *Am Ind Hyg Assoc J* 1998; 59(2): 128-32. [<http://dx.doi.org/10.1080/15428119891010389>] [PMID: 9487666]
- [17] Clifton W, Damon A, Martin AK. Considerations and cautions for three-dimensional-printed personal protective equipment in the COVID-19 crisis. *3D Printing and Additive Manufacturing* 2020; 7(3): 97-.
- [18] Covid-19 response. National Institutes of Health. US Department of Health and Human Services 2022. <https://3dprint.nih.gov/collections/covid-19-response>
- [19] Iannace S, Sorrentino L, Di Maio E. Biodegradable biomedical foam scaffolds. *Biomedical Foams for Tissue Engineering Applications* 2014; pp. 163-87.
- [20] J Parry E, Banks CE. Covid-19: Additive manufacturing response in the UK. *Journal of 3D Printing in Medicine* 2020; 4(3): 167-74.
- [21] List N Advanced Search Page. Disinfectants for Coronavirus (COVID-19) EPA Environmental Protection Agency 2022. <https://www.epa.gov/pesticide-registration/list-n-advanced-search-page-disinfectants-coronavirus-covid-19>
- [22] Infection prevention and control of epidemic-and pandemic prone acute respiratory infections in health care.. World Health Organization

- World Health Organization  
2022. <https://www.who.int/publications/i/item/infection-prevention-and-control-of-epidemic-and-pandemic-prone-acute-respiratory-infections-in-health-care>
- [23] Cleaning and disinfection of environmental surfaces in the context of covid-19: Interim guidance, 15 May 2020.. World Health Organization  
World Health Organization  
1970. <https://apps.who.int/iris/handle/10665/332096>
- [24] Mask fitter by Bellus3D. National Institutes of Health.. US Department of Health and Human Services  
2022. <https://3dprint.nih.gov/discover/3dpx-013836>
- [25] Liu J, Ma J, Ahmed IK, Varma DK. Effectiveness of a 3D-printed mask fitter in an ophthalmology setting during COVID-19. *Canadian Journal of Ophthalmology* 2021.
- [26] Kim Y, Yoon C, Ham S, *et al.* Emissions of nanoparticles and gaseous material from 3D printer operation. *Environ Sci Technol* 2015; 49(20): 12044-53.  
[<http://dx.doi.org/10.1021/acs.est.5b02805>] [PMID: 26402038]
- [27] Schraufnagel DE. The health effects of ultrafine particles. *Exp Mol Med* 2020; 52(3): 311-7.  
[<http://dx.doi.org/10.1038/s12276-020-0403-3>] [PMID: 32203102]
- [28] Chan FL, House R, Kudla I, Lipszyc JC, Rajaram N, Tarlo SM. Health survey of employees regularly using 3D printers. *Occup Med (Lond)* 2018; 68(3): 211-4.  
[<http://dx.doi.org/10.1093/occmed/kqy042>] [PMID: 29538712]
- [29] Bernard M, Jubeli E, Pungente MD, Yagoubi N. Biocompatibility of polymer-based biomaterials and medical devices – regulations, in vitro screening and risk-management. *Biomaterials Science* 6(8): 2025-53.
- [30] Bussan DD, Snaychuk L, Bartzas G, Douvris C. Quantification of trace elements in surgical and KN95 face masks widely used during the SARS-COVID-19 pandemic. *Science of The Total Environment* 24: 151924.
- [31] Sethurajan M, Lens PN, Horn HA, Figueiredo LH, van Hullebusch ED. Leaching and recovery of metals. *Sustainable Heavy Metal Remediation* 161-206.  
[[http://dx.doi.org/10.1007/978-3-319-61146-4\\_6](http://dx.doi.org/10.1007/978-3-319-61146-4_6)]
- [32] Chohan JS, Singh R. Pre and post processing techniques to improve surface characteristics of FDM parts: A State of Art Review and Future Applications. *Rapid Prototyping J* 23(3): 495-513.  
[<http://dx.doi.org/10.1108/RPJ-05-2015-0059>]

© 2022 Amir and Amir.

This is an open access article distributed under the terms of the Creative Commons Attribution 4.0 International Public License (CC-BY 4.0), a copy of which is available at: <https://creativecommons.org/licenses/by/4.0/legalcode>. This license permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited.